BIOVIRIDIAN

Excellence in HPLC-MS Analysis

CERTIFICATE OF ANALYSIS

Sample Received: **February 18, 2026** COA Issued: **February 24, 2026**

PRODUCT INFORMATION

Vendor: **Bionic Labs**

Sample Name: **BPC-157, with TB-500 10mg**

Sample Type: **White lyophilized powder**

Batch Number: **26110**

MW: **1419, & 4964 g/mol**

ANALYTICAL METHODS


Identity: Confirmed via MALDI–MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation


TEST RESULTS

Specification	Result	Method	Status
Identity: BPC-157, with TB-500	BPC-157, & TB-500	MALDI-MS	✓ Conforms
Content	5.13, 5.24 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms


ANALYTICAL DATA

HPLC Chromatogram (Retention Time: 5.967, & 5.783 **min)**

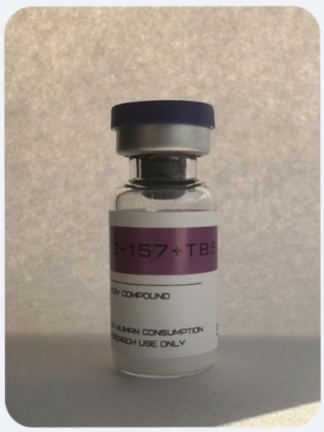

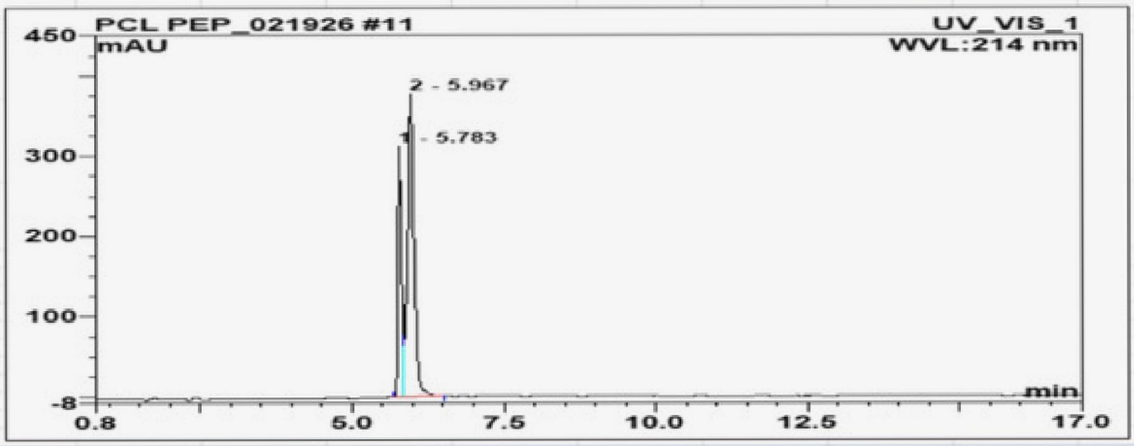

Mass Spectrum (MALDI-MS)

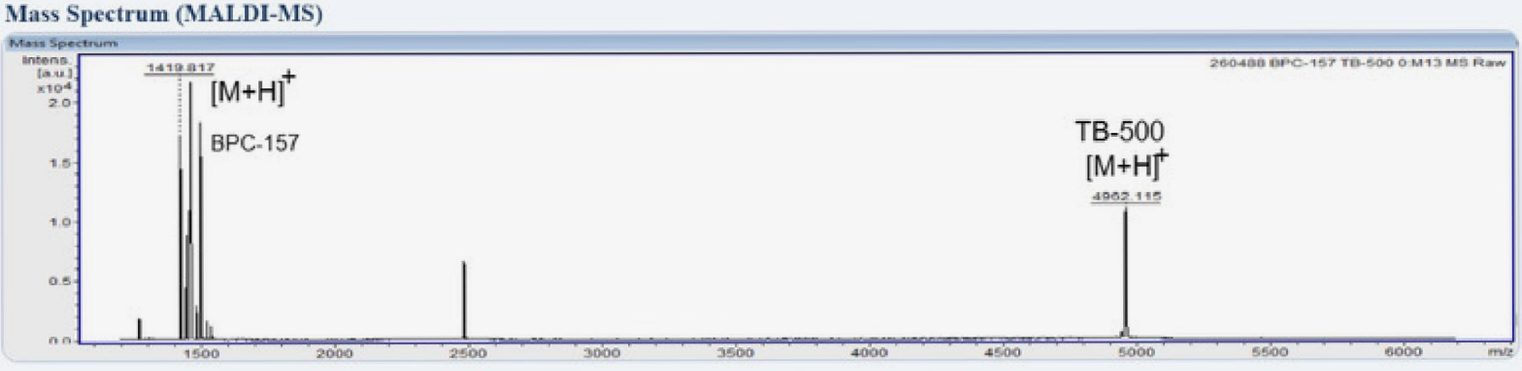

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.